


Group OrgLab

C13\_H1dec.UW CDCl3 /home/chem344/ay400 chem344 77

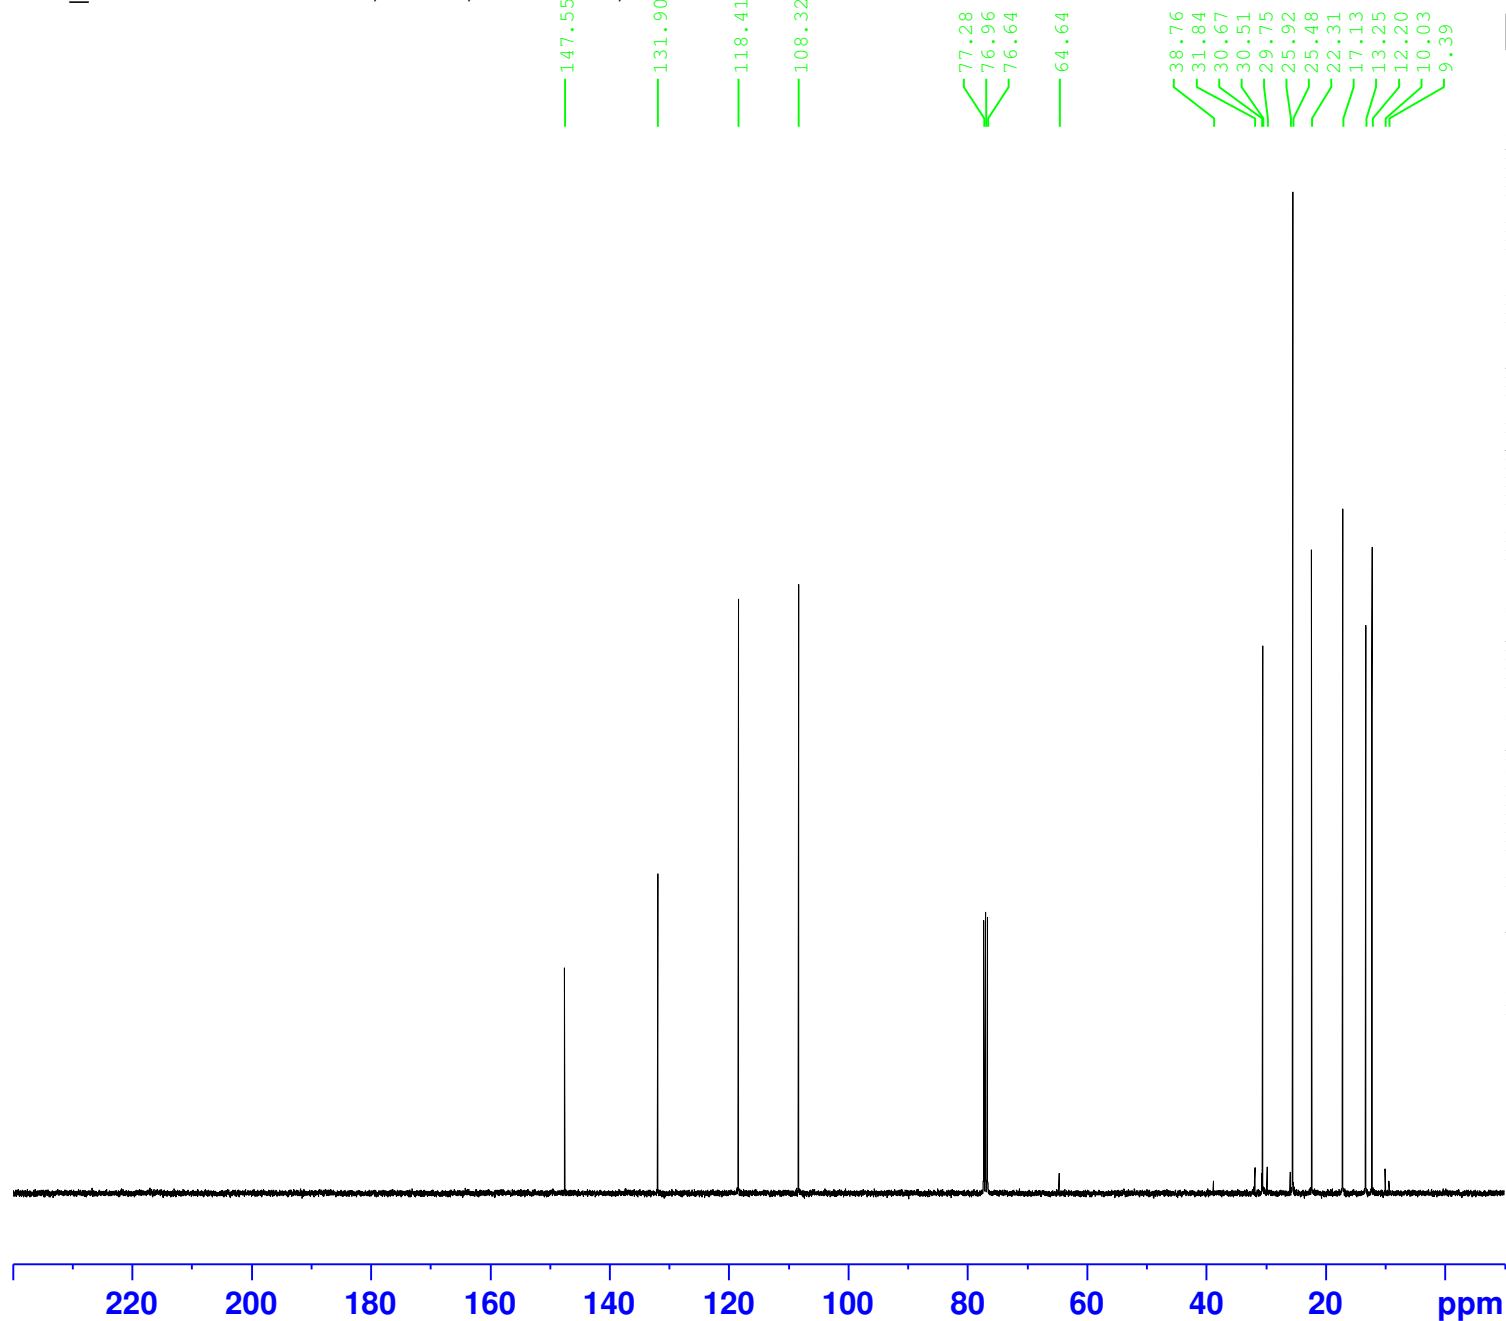

Current Data Parameters  
NAME CHEM 344 E2 Product Mixture  
EXPNO 12  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20180313  
Time 8.12  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgpg30  
TD 71424  
SOLVENT CDCl3  
NS 128  
DS 2  
SWH 28409.092 Hz  
FIDRES 0.397753 Hz  
AQ 1.2570624 sec  
RG 193.02  
DW 17.600 usec  
DE 6.50 usec  
TE 297.2 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6364098 MHz  
NUC1 13C  
P1 10.00 usec  
PLW1 52.00000000 W

===== CHANNEL f2 =====  
SFO2 400.1818008 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 10.72000027 W  
PLW12 0.29778001 W  
PLW13 0.24120000 W

F2 - Processing parameters  
SI 65536  
SF 100.6253410 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40